

1           **TESTING SEEDS PROTECTED WITH AN INSECTICIDE**

2                           **BY NEAR INFRARED SPECTROSCOPY**

3  
4                           Pierre Billen<sup>1</sup>, Olivier Pigeon<sup>2</sup>, and Pierre Dardenne<sup>1</sup>

5  
6           <sup>1</sup> CRAGx, Département Qualité des Productions Agricoles, Chaussée de Namur 24, B-5030 Gembloux (Belgium).

7           <sup>2</sup> CRAGx, Département Phytopharmacie, Rue du Bordia 11, B-5030 Gembloux (Belgium).

8  
9           Keywords : crop protection, treated seeds, insecticide, Tefluthrin, Austral Plus, NIRS

10  
11           **SUMMARY**

12           Near Infrared Spectroscopy (NIR) was evaluated to analyse seeds treated with a  
13           formulation containing an insecticide : Tefluthrin. Tefluthrin is an active ingredient  
14           present in Austral Plus, used to protect wheat seeds. The main objectives of the project are  
15           the determination of the average concentration of Tefluthrin in seed batches and the study  
16           of the distribution of Tefluthrin among individual seeds. Two different sample  
17           presentations were used to solve these questions : the "bulk presentation" and the "single-  
18           seed presentation".

19           Calibrations were developed to quantify the average concentrations ( $R^2 = 0.97$ ,  
20           SD/SEC = 6.0) as well as to determine the uniformity of the insecticide ( $R^2 = 0.85$ ,  
21           SD/SEC = 2.6) in batches of seeds. The first model is more accurate but both produce  
22           satisfactory results.

23 **INTRODUCTION**

24 It is commonplace in agricultural practice to use seeds treated with plant protection  
25 product. The purpose of the present research is to develop a quick method for monitoring  
26 batches of seeds, to identify the active ingredient in the coating as well as to determine its  
27 concentration and its uniformity. Being a fast and non-destructive technique, Near  
28 Infrared Spectroscopy seems to be well suited to solve these questions. The aim of this  
29 work is to establish equations to analyse Tefluthrin, an active ingredient present in Austral  
30 Plus, product used to protect wheat seeds.

31 Tefluthrin is an insecticide of the family of Pyrethroids. It controls a wide range of  
32 soil insect pests, particularly those of the orders Coleoptera, Lepidoptera and Diptera. This  
33 active ingredient is solid at ambient temperature. It is soluble in acetone, hexane, toluene,  
34 dichloromethane, ethyl acetate and methanol. After extraction in one of these solvents,  
35 Tefluthrin is analysed by gas chromatography.<sup>1</sup>

36 Tefluthrin is one of the three active ingredients of Austral Plus. The composition of  
37 Austral Plus is 40 g L<sup>-1</sup> Tefluthrin, 60 g L<sup>-1</sup> Anthraquinone (a bird repellent, in particular  
38 rooks) and Fludioxonil (a fungicide). Austral Plus is usually used at the dose of 500 ml kg<sup>-1</sup>  
39 of wheat seeds.<sup>1</sup>

40 **MATERIALS AND METHODS**

41

42 **Chemical Determinations**

43 Tefluthrin was extracted by acetone during 90 min in an ultrasonic bath. Tefluthrin  
44 in solution was analysed by gas chromatography (Hewlett-Packard 6890 Series with an  
45 Electron Capture Detector ( $^{63}\text{Ni}$ ) -ECD- or with a Flame Ionisation Detector -FID-) using  
46 the external standard calibration.<sup>2,3</sup>

47 To determine average concentrations in the batches, Tefluthrin was extracted from  
48 35, 50 and 65 seeds with 50 ml acetone. The concentration on one single seed is  
49 determined after an extraction with 5 ml acetone.<sup>2,3</sup>

50

51 **Acquisition of the spectra, data processing**

52 The seed spectra were acquired in reflection mode on a NIRSystems 6500 (Foss-  
53 NIRSystems Inc., Silver Spring, MD, USA) spectrometer. This monochromator is able to  
54 collect spectral data from 400 to 2500 nm in steps of 2 nm.

55 We have been using two types of sample presentation: the "bulk presentation" to  
56 determine average concentrations in the batches of seeds, and the "single-seed  
57 presentation" to characterise the distribution of Tefluthrin among individual seeds.

58 In the "bulk presentation", the cell is rectangular and can contain 100 g of seeds.  
59 During the measurement, the cell is stopping at 32 different places. The result is the  
60 average of 32 spectra. In the "single-seed presentation", the seed is measured in a rotating  
61 drawer. The cell is equipped with a full aluminium disc with a cavity in its middle where  
62 the seed is placed. During the spectral analysis, the cell is turning and the sample is also  
63 measured at different places. In the two cases, each sample is measured in duplicate.

64 The spectrum of pure Austral Plus was acquired in transmission mode. The  
65 pathlength of the used cell is 0.5 mm. Due to the small available quantity of Tefluthrin, its  
66 spectrum was acquired in reflexion mode on a AutoIMAGE Microscope connected to a  
67 Perkin-Elmer FT-NIR.

68 The spectral data were treated with the ISI-NIRS 3 ver. 4.0 software (Foss-Infrasoft  
69 International, Port Matilda, PA, USA).<sup>4,5</sup> The calibration was obtained by a modified  
70 Partial Least Squares (MPLS) regression technique as available in the ISI package.<sup>4,5</sup> This  
71 technique is the classical PLS<sup>6</sup> algorithm with a standardisation of the X residuals at each  
72 iteration.<sup>7</sup> This regression technique requires cross-validation to prevent overfitting. Cross  
73 validation estimates calibration performances by partitioning the calibration set into  
74 several groups.<sup>7</sup> The ISI software allows calibrations on the basis of raw spectra, of their  
75 first or their second derivatives as well as baseline correction.<sup>4,5</sup> Trials and errors is the  
76 only way to get the best analytical performances.<sup>5</sup> The latter are characterized by the  
77 standard error of calibration (SEC), the determination coefficient of calibration (RSQ), the  
78 standard error of cross validation (SECV) and the determination coefficient of cross  
79 validation (RSQV). A ratio SD/SEC (SD = standard deviation of the population) of more  
80 than 3.0 is required for quantitative determination. The higher this value the more accurate  
81 the model is.<sup>8</sup>

82

### 83 **Sampling**

84 The seed batches were supplied by the Belgian Ministry of Small Enterprises,  
85 Traders and Agriculture. Moreover, thirty batches were treated with accurately known  
86 quantities of Austral Plus to get a rectangular distribution.

87 For the bulk determinations, ninety eight batches of wheat seeds were investigated  
88 to build the calibration to estimate the average concentration. For the single seed  
89 determinations, 630 seeds within 42 batches were selected for calibration and for testing  
90 the homogeneity within the batches.

91

## 92 **RESULTS AND DISCUSSION**

93

### 94 **Raw Spectra**

95 Before calibration, it is interesting to study the raw spectra. Figure 1 shows  
96 specific absorbance bands of Tefluthrin which are clearly recognisable in the spectrum of  
97 Austral Plus and two treated wheat seed batches. As expected, higher peaks in the spectra  
98 of treated seed batches correspond to larger quantities of Austral Plus. Some wavelengths  
99 (1654-1666, 1944-1954, 2142-2152, 2254-2260, 2308- 2312, 2360- 2368, 2442-2446 nm)  
100 are common to the spectra of Tefluthrin, Austral Plus and treated batches.

101

### 102 **Calibrations**

103 Figures 1 and 2 show the two scatter plots of the regression to predict (1) average  
104 concentrations and (2) distribution of treatment in batches of seeds. The wavelengths from  
105 400 nm to 700 nm (visible range) were not used in developing the equations. The two  
106 databases were searched for outliers using the Mahalanobis distances (H statistic). Three  
107 samples in the first database (for bulk determinations) and five in the second database (for  
108 single-seed determinations) with H values higher than three were discarded to avoid  
109 singular samples. In the second database, thirty samples with very low concentrations of  
110 Tefluthrin were discarded.

111 In both cases, the best treatment of the spectral data is 2, 5, 5 (2 for the second  
112 derivative, 5 for the subtraction gap and the smoothing segment expressed in data points,  
113 respectively) without any scatter correction. The number of cross validation groups is six  
114 in the first database and four in the second database. During the calibration five samples of  
115 the first database (5.1 % of the population) and twenty-six of the second database (4,4 %  
116 of the population) were discarded owing to too high residual values. The two calibrations  
117 (Table 1) are acceptable but the equation to determine the average concentrations of  
118 Tefluthrin is better than the other one (SD/SEC = 5.99 vs 2.61; RSQ = 0.97 vs 0.85). The  
119 bulk absorbances are stronger than single seed ones as the instrument design has not been  
120 modified to focus the light beam on the single seed.

121

## 122 **CONCLUSIONS**

123 The NIR technique may be used to predict the active ingredient Tefluthrin. The  
124 bulk as well as the single seed measurement yield satisfactory results. The average  
125 concentration of Tefluthrin in batches of wheat seeds can be obtained with a good  
126 accuracy on the basis of bulk measurements. The single seed measurements allow a good  
127 estimate of the distribution of Tefluthrin within seed batches. In the future, it would be  
128 interesting to build models for other active ingredients and thus other important products  
129 used for coating other seeds. A similar approach is currently developed to predict  
130 Imidacloprid which is an active ingredient in Gaucho, a product used to protect barley  
131 seeds.

132

## 133 **ACKNOWLEDGEMENTS**

134           We would like to thank DG4 (Inspection of Raw Materials Belgian Ministry of  
135 Small Enterprises, Traders and Agriculture) for their financial support.

136 **REFERENCES**

137

- 138 1. British Crop Protection Council, in *The Pesticide Manual, 11th Edition*, Ed by CDF  
139 Tomlin. UK, pp. 48-50, 566-568, 1160-1161 (1997).
- 140 2. H. Braunschweig, H.-G. Nolthing, J. Siebees and H.Köhle, *Manual of Pesticide*  
141 *Residue Analysis, Volume II, Multi-residue Method S 23*, Ed by H.-P. Thier and J.  
142 Kirchhoff. Pesticides Commission, Germany, pp. 333-342 (1992).
- 143 3. Working Group "Ontwikkeling van Residu-analysemethoden". *Analytical Methods for*  
144 *Pesticide Residues in Foodstuffs, 6th Edition, Part I, Multi-residue Method 1*, General  
145 Inspectorate for Health Protection, Ministry of Public Health, Welfare and Sport. The  
146 Netherlands, pp. 1-22 (1996).
- 147 4. J.S. Shenk and M.O. Westerhaus, *ISI-NIRS 3.0 Manual*, Infracsoft International, Port  
148 Matilda, PA, USA, pp. 331 (1992).
- 149 5. J.S. Shenk and M.O. Westerhaus, *Monograph: Analysis of Agriculture and Food*  
150 *Products by Near Infrared Reflectance Spectroscopy*, Infracsoft International, Port  
151 Matilda, PA, USA, p. 103 (1993).
- 152 6. S. Wold, A. Ruhe, H. Wold and W. Dunn, *Siam J. of Sci. and Stats. Comput.* **5**, 735-  
153 743 (1984).
- 154 7. G. Sinnaeve, P. Dardenne and R. Agneessens, *J. Near Infrared Spectrosc.* **2**, 163-175  
155 (1994).
- 156 8. P. Williams and D. Sobering, in *Proc. of the 5th ICNIRS, Haugesund (Norway)*, Ed by  
157 K.I. Hildrun, T.Isaksson, T.Naes and A.Tandberg, Ellis Horwood, Chichester, pp. 441-  
158 446 (1992).



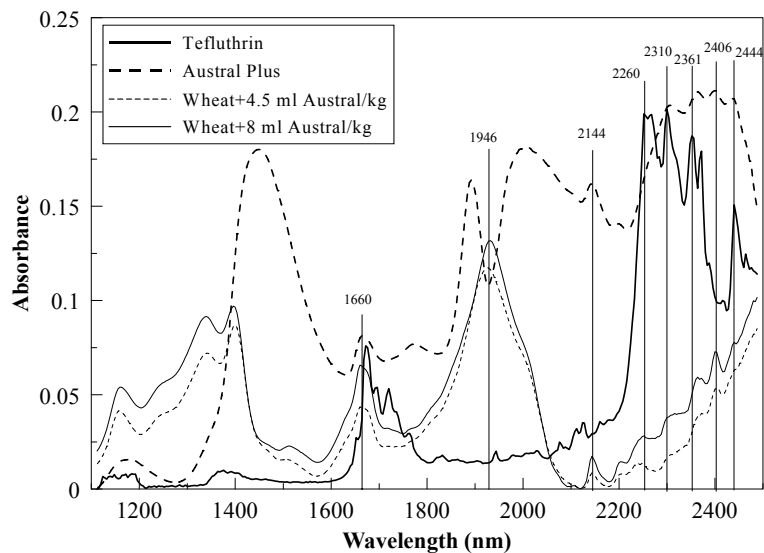


Figure 1. Spectra of Tefluthrin, Austral Plus and two batches of wheat seeds treated at two levels with Austral Plus.

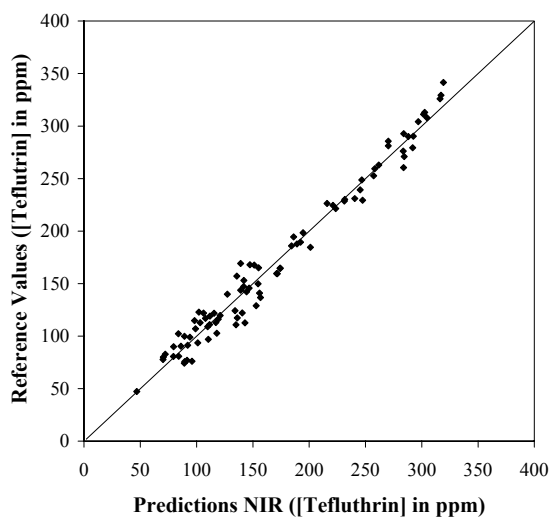


Figure 2. Scatter plots of the regression to predict average concentrations of treatment in batches of seeds.

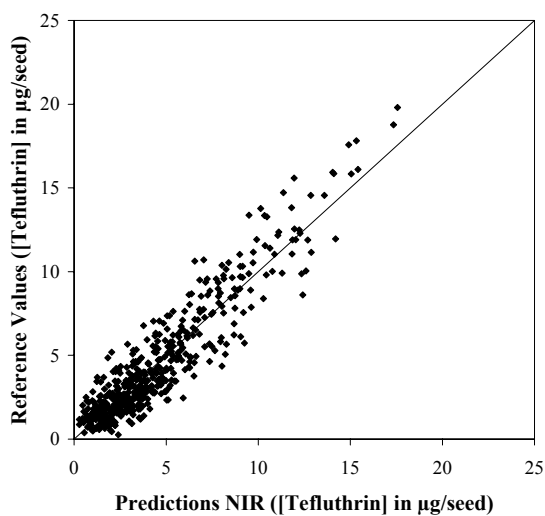


Figure 3. Scatter plots of the regression to predict distribution of treatment in batches of seeds.

Table 1. Performance of equations to predict (1) average concentrations and (2) the distribution of the single seed treatment.

	N	Range	Mean	SD	SEC	SD/SEC	RSQ	SECV	RSQV	PLST
Tefluthrin (ppm)	90	47.3 - 341.6	170.8	76.94	12.85	5.99	0.97	18.80	0.94	7
Tefluthrin (µg/seed)	569	0.31 - 19.80	4.29	3.445	1.32	2.61	0.85	1.56	0.80	12

N: Number of Samples

SEC: Standard Error of Calibration

SECV: Standard Error of Cross Validation

PLST: Number of PLS Terms

SD: Standard Deviation

RSQ: Determination coefficient of Calibration

RSQV: Determination coefficient of Cross Validation